


- Ammonia (NH3 as N), FIL, DA -
Blind Blank Results
Lab: NWQL, PCode: 00608, MCode: SHC02
Analysis dates: 10/01/14 through 06/28/19
[Open Data Set](#)

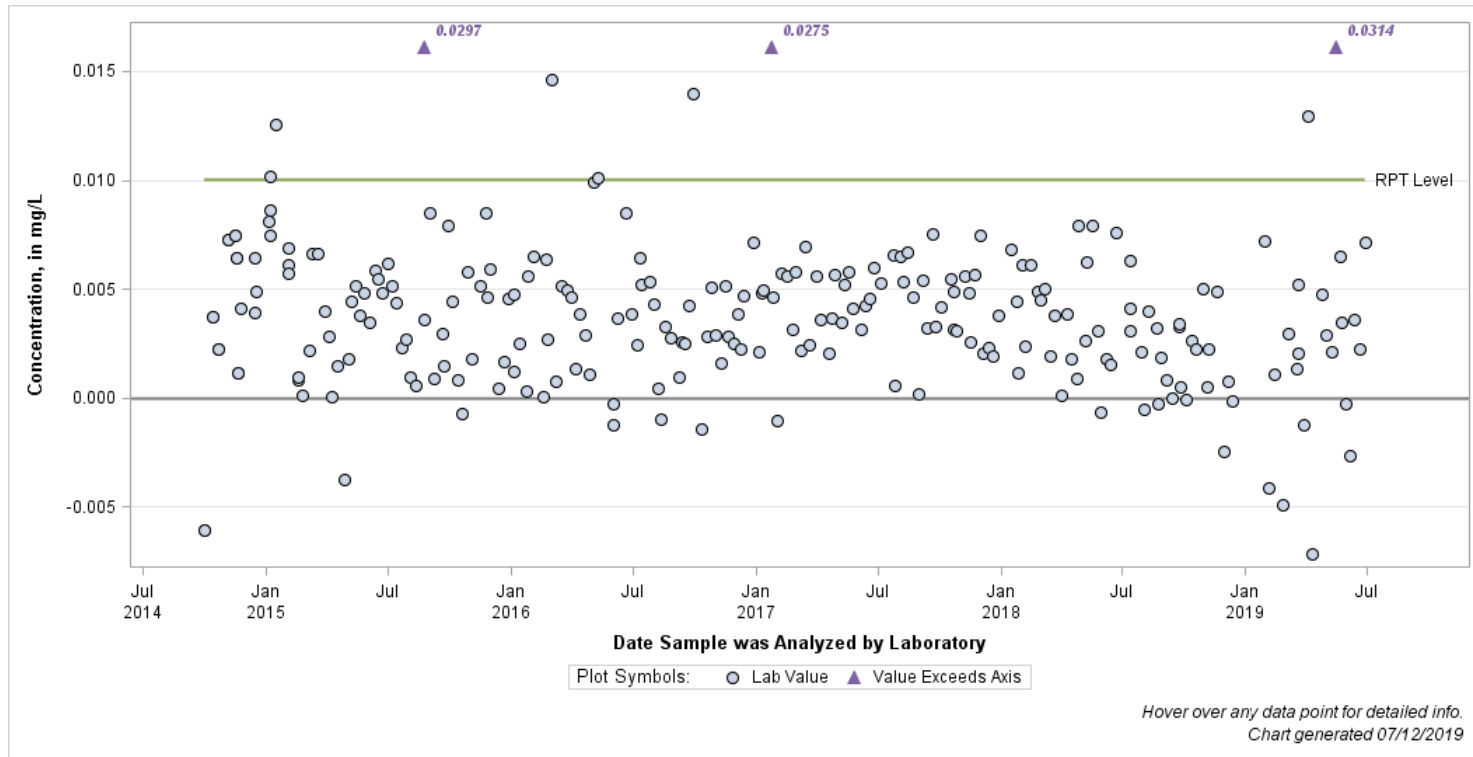


False Positive Rate for Ammonia (NH3 as N), FIL, DA

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Ammonia (NH3 as N), FIL, DA	00608SHC02	2014	2	0	0%
		2015	58	3	5%
		2016	51	3	6%
		2017	51	1	2%
		2018	51	0	0%
		2019	32	2	6%

**Highlighted if false positive rate > 5%*

Hover over any data point for detailed info.
Chart generated 07/12/2019

- Ammonia (NH3 as N), UNF, CFA, Acidified -
Blind Blank Results
Lab: NWQL, PCode: 00610, MCode: CL017
Analysis dates: 05/08/15 through 06/10/19
[Open Data Set](#)

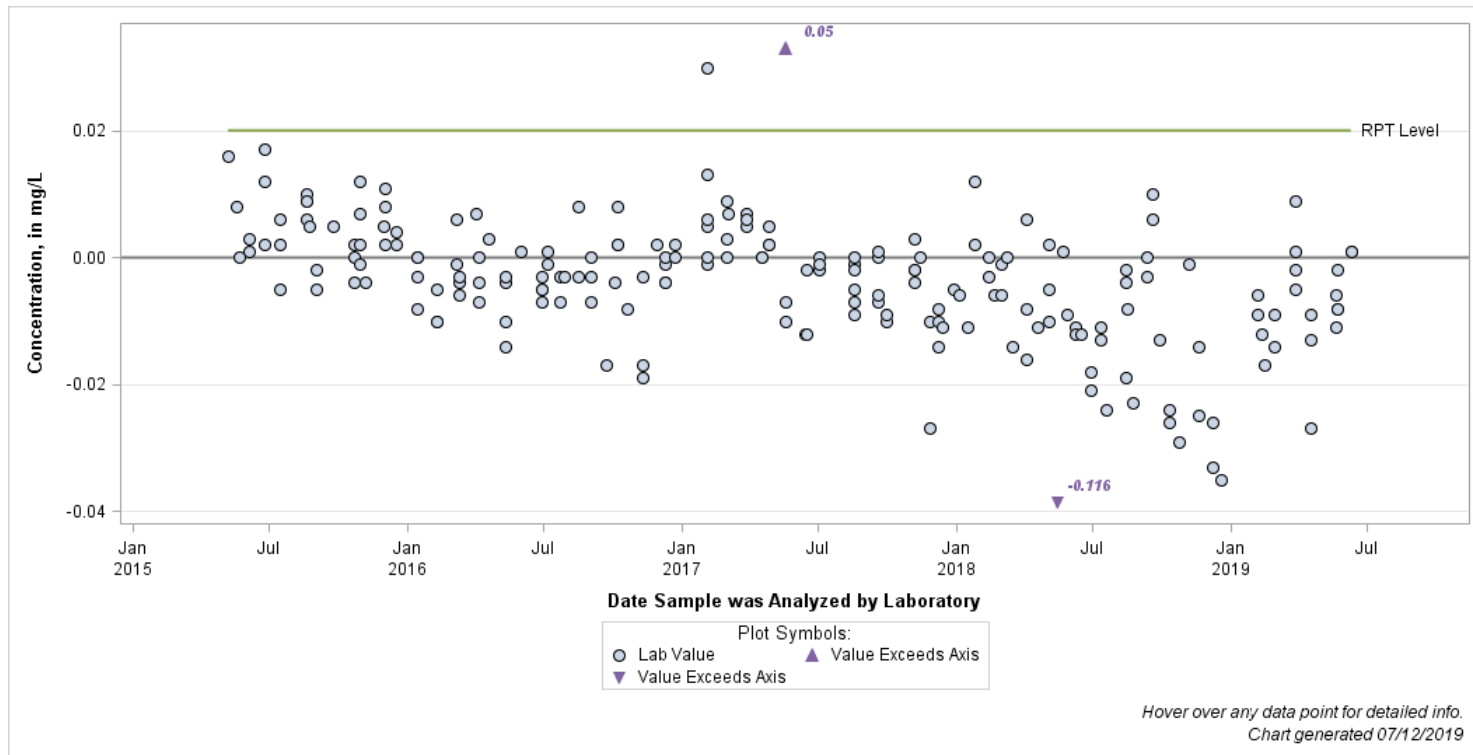


False Positive Rate for Ammonia (NH3 as N), UNF, CFA, Acidified

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Ammonia (NH3 as N), UNF, CFA, Acidified	00610CL017	2015	22	0	0%
		2016	51	0	0%
		2017	51	2	4%
		2018	51	0	0%
		2019	29	0	0%

*Highlighted if false positive rate > 5 %

Hover over any data point for detailed info.
 Chart generated 07/12/2019

- Kjeldahl Nitrogen (NH₃+org N as N), FIL, CFA -
Blind Blank Results
Lab: NWQL, PCode: 00623, MCode: KJ002
Analysis dates: 10/03/14 through 06/20/19
[Open Data Set](#)

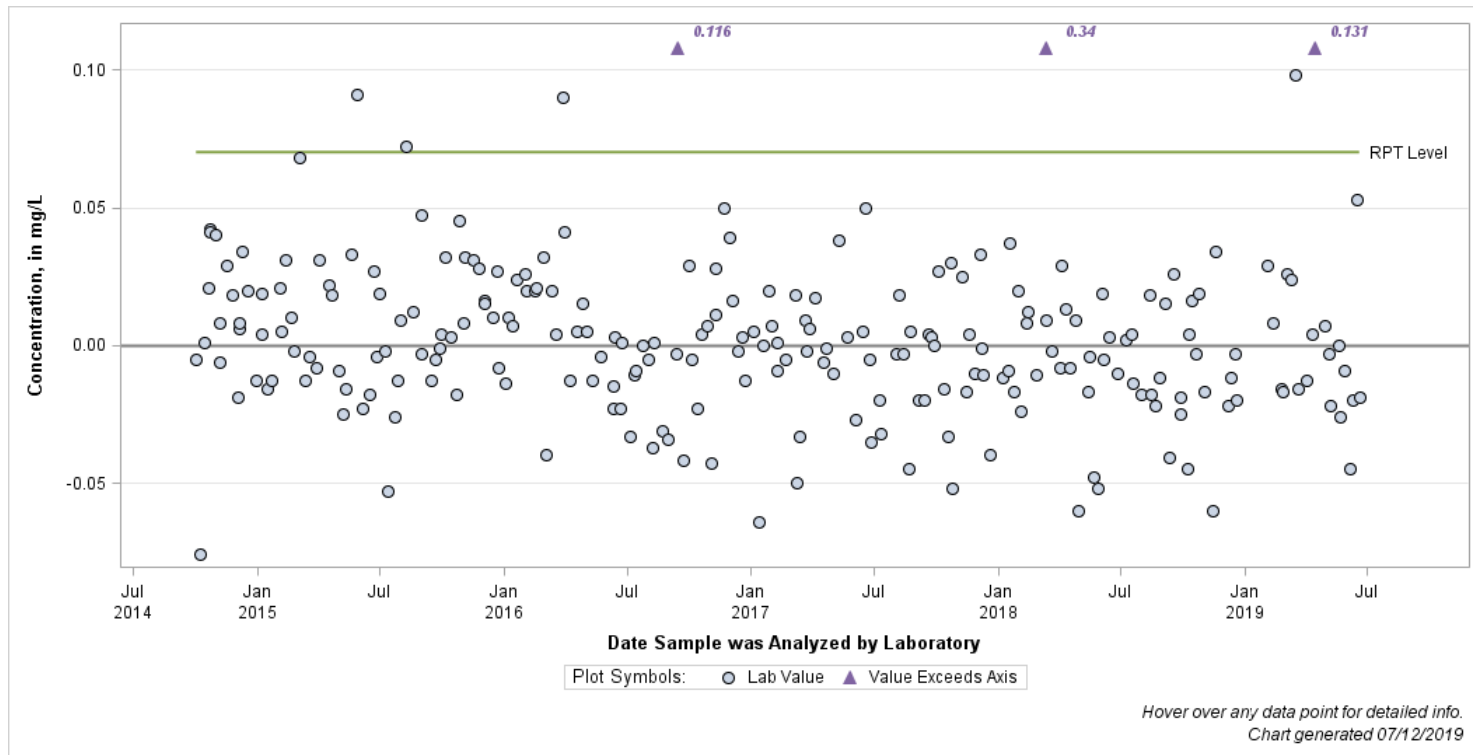

False Positive Rate for Kjeldahl Nitrogen (NH₃+org N as N), FIL, CFA

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Kjeldahl Nitrogen (NH ₃ +org N as N), FIL, CFA	00623KJ002	2014	5	0	0%
		2015	52	2	4%
		2016	51	2	4%
		2017	51	0	0%
		2018	51	1	2%
		2019	32	2	6%

*Highlighted if false positive rate > 5 %

Hover over any data point for detailed info.
Chart generated 07/12/2019


- Kjeldahl Nitrogen (NH3+org N as N), UNF, CFA, ACD -

Blind Blank Results

Lab: NWQL, PCode: 00625, MCode: KJ008

Analysis dates: 10/06/14 through 06/06/19

[Open Data Set](#)

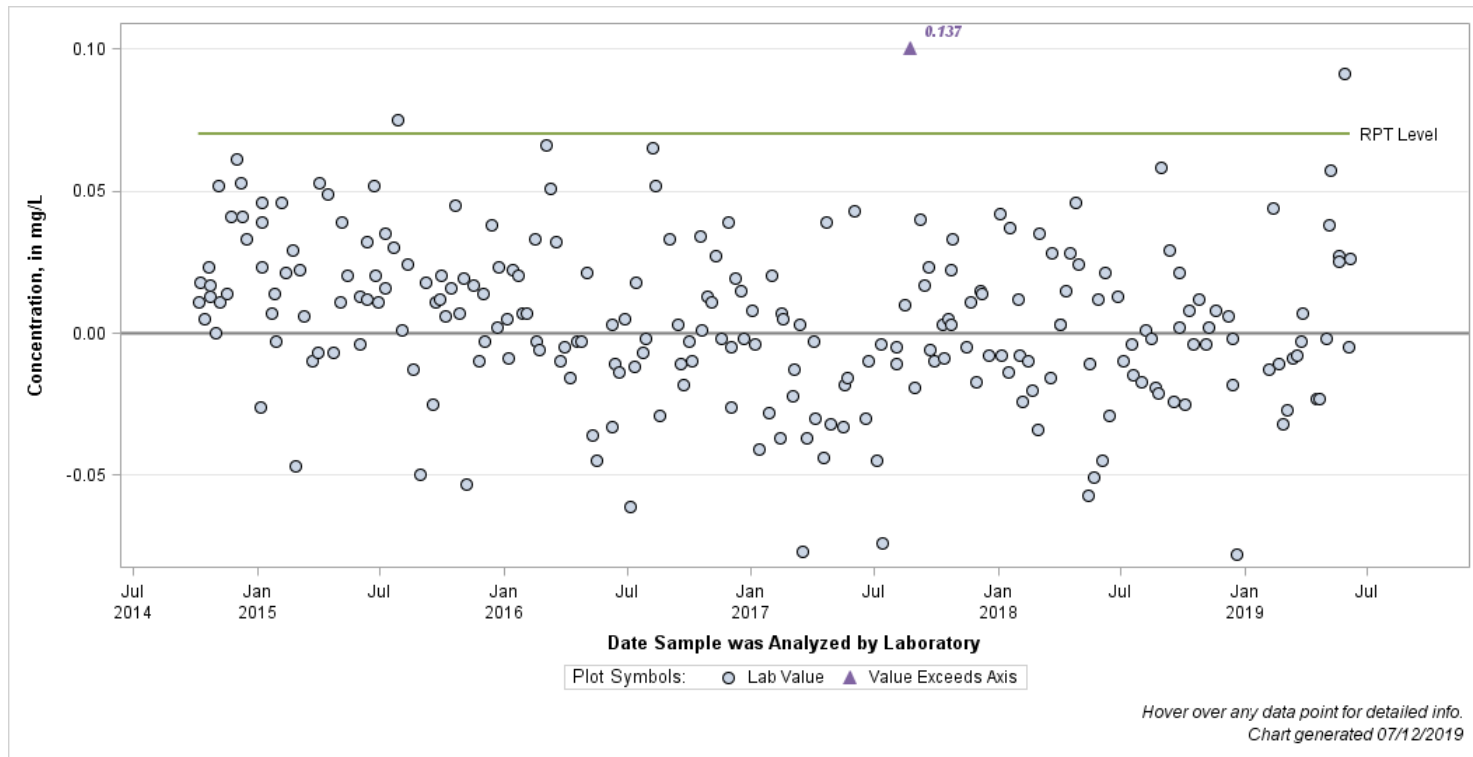

False Positive Rate for Kjeldahl Nitrogen (NH3+org N as N), UNF, CFA, ACD

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Kjeldahl Nitrogen (NH3+org N as N), UNF, CFA, ACD	00625KJ008	2014	5	0	0%
		2015	52	1	2%
		2016	51	0	0%
		2017	51	1	2%
		2018	51	0	0%
		2019	29	1	3%
		*Highlighted if false positive rate > 5 %			

Hover over any data point for detailed info.
Chart generated 07/12/2019


- Nitrate plus Nitrite (NO3+NO2 as N), FIL, DA -

Blind Blank Results

Lab: NWQL, PCode: 00631, MCode: RED01

Analysis dates: 10/02/14 through 06/26/19

[Open Data Set](#)

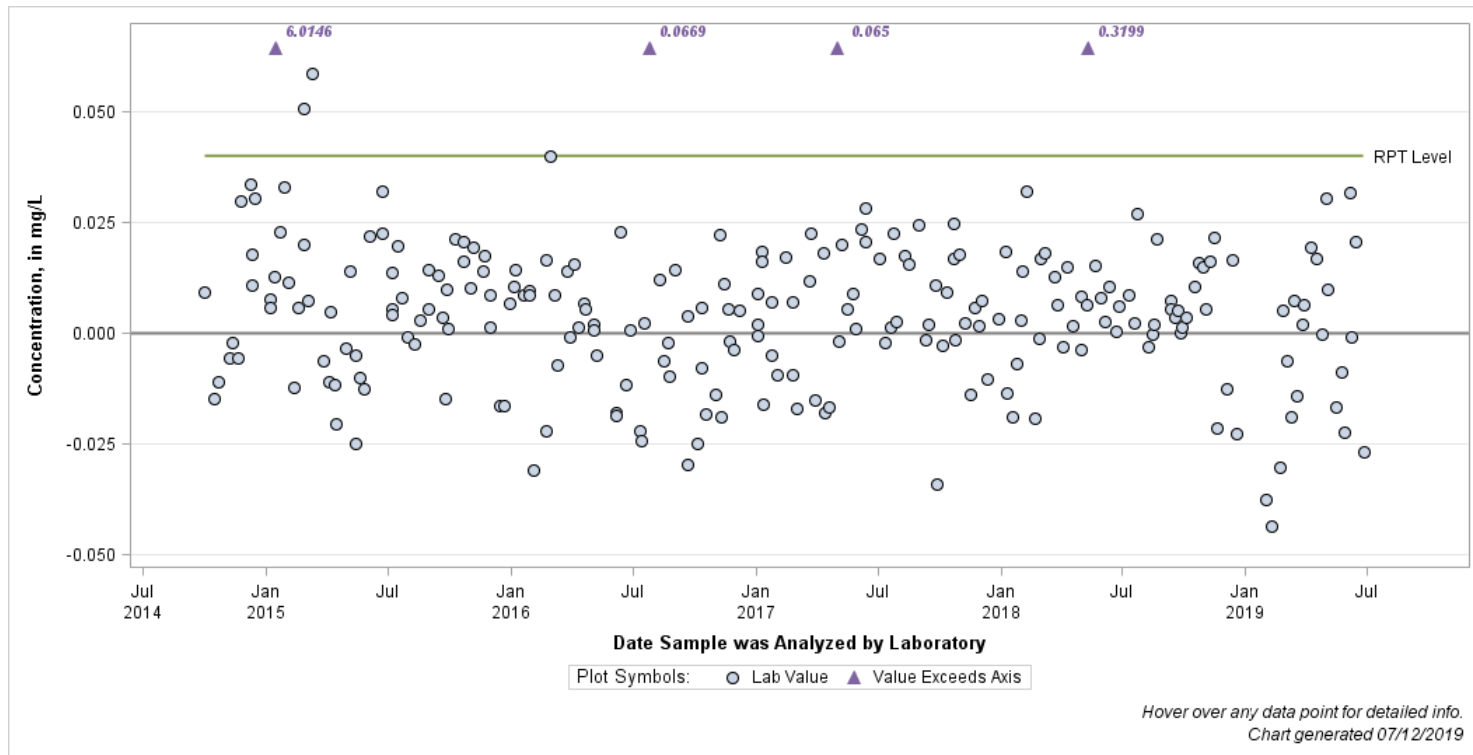

False Positive Rate for Nitrate plus Nitrite (NO3+NO2 as N), FIL, DA

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Nitrate plus Nitrite (NO3+NO2 as N), FIL, DA	00631RED01	2014	1	0	0%
		2015	52	3	6%
		2016	51	1	2%
		2017	51	1	2%
		2018	51	1	2%
		2019	32	0	0%

*Highlighted if false positive rate > 5%

Hover over any data point for detailed info.
Chart generated 07/12/2019


- Nitrate plus Nitrite (NO3+NO2 as N), FIL, DA, LL -

Blind Blank Results

Lab: NWQL, PCode: 00631, MCode: RED02

Analysis dates: 10/07/14 through 06/20/19

[Open Data Set](#)

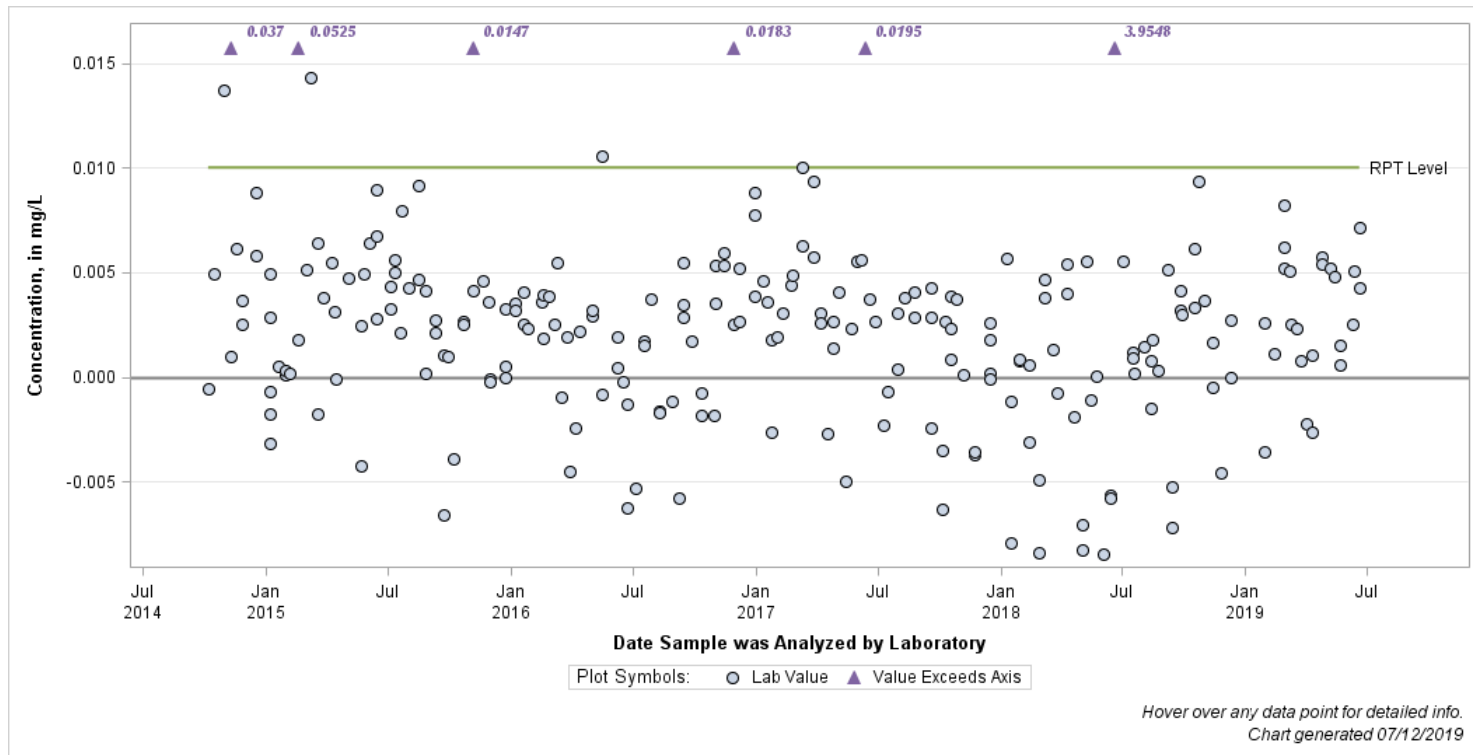


False Positive Rate for Nitrate plus Nitrite (NO3+NO2 as N), FIL, DA, LL

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Nitrate plus Nitrite (NO3+NO2 as N), FIL, DA, LL	00631RED02	2014	1	0	0%
		2015	52	4	8%
		2016	51	2	4%
		2017	51	3	6%
		2018	51	1	2%
		2019	32	0	0%

*Highlighted if false positive rate > 5 %

Hover over any data point for detailed info.
Chart generated 07/12/2019

- Nitrite (NO2 as N), FIL, DA -
Blind Blank Results
Lab: NWQL, PCode: 00613, MCode: DZ001
Analysis dates: 10/01/14 through 06/28/19
[Open Data Set](#)

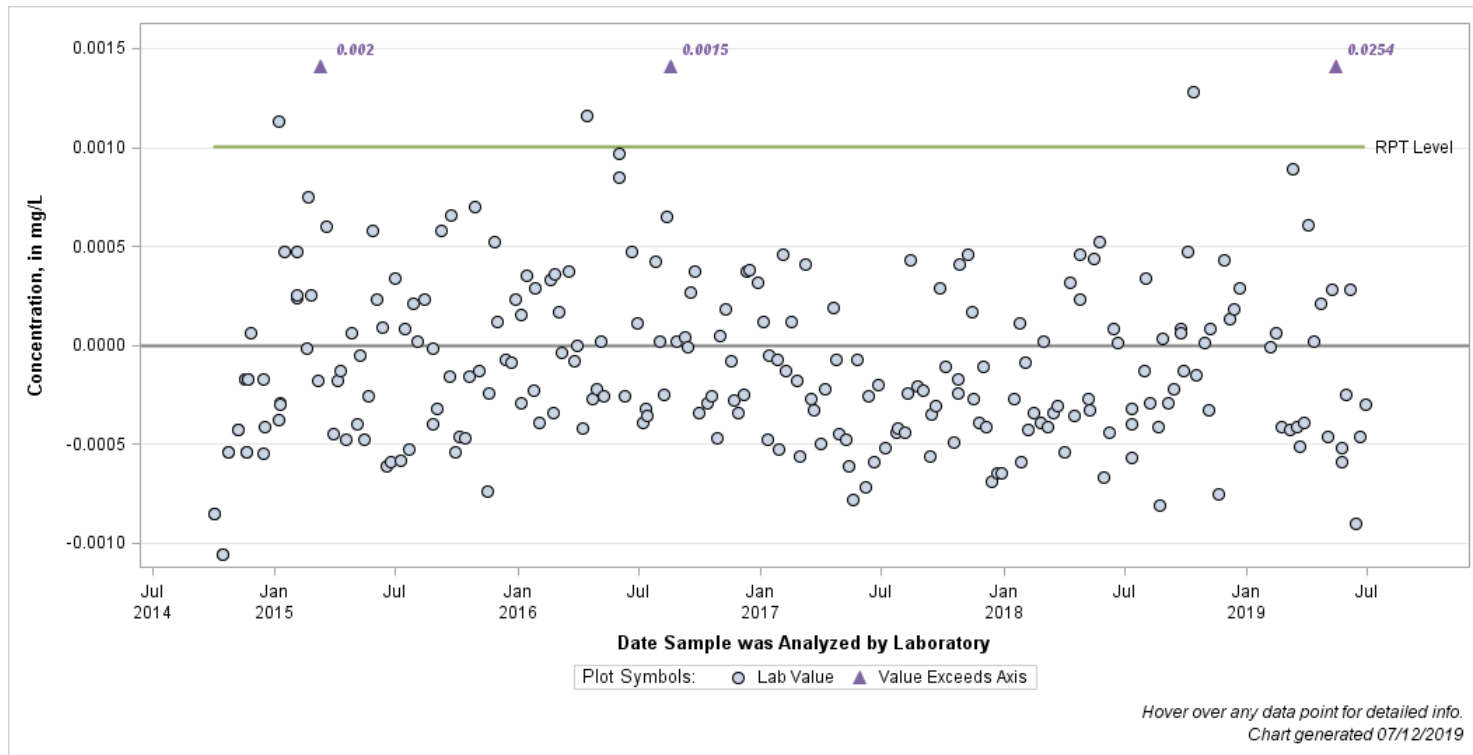


False Positive Rate for Nitrite (NO2 as N), FIL, DA

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Nitrite (NO2 as N), FIL, DA	00613DZ001	2014	2	0	0%
		2015	58	2	3%
		2016	51	2	4%
		2017	51	0	0%
		2018	51	0	0%
		2019	32	2	6%

**Highlighted if false positive rate > 5 %*

*Hover over any data point for detailed info.
Chart generated 07/12/2019*

**- Orthophosphate (PO4 as P), FIL, DA -
Blind Blank Results**
Lab: NWQL, PCode: 00671, MCode: PHM01
Analysis dates: 10/08/14 through 06/28/19
[Open Data Set](#)

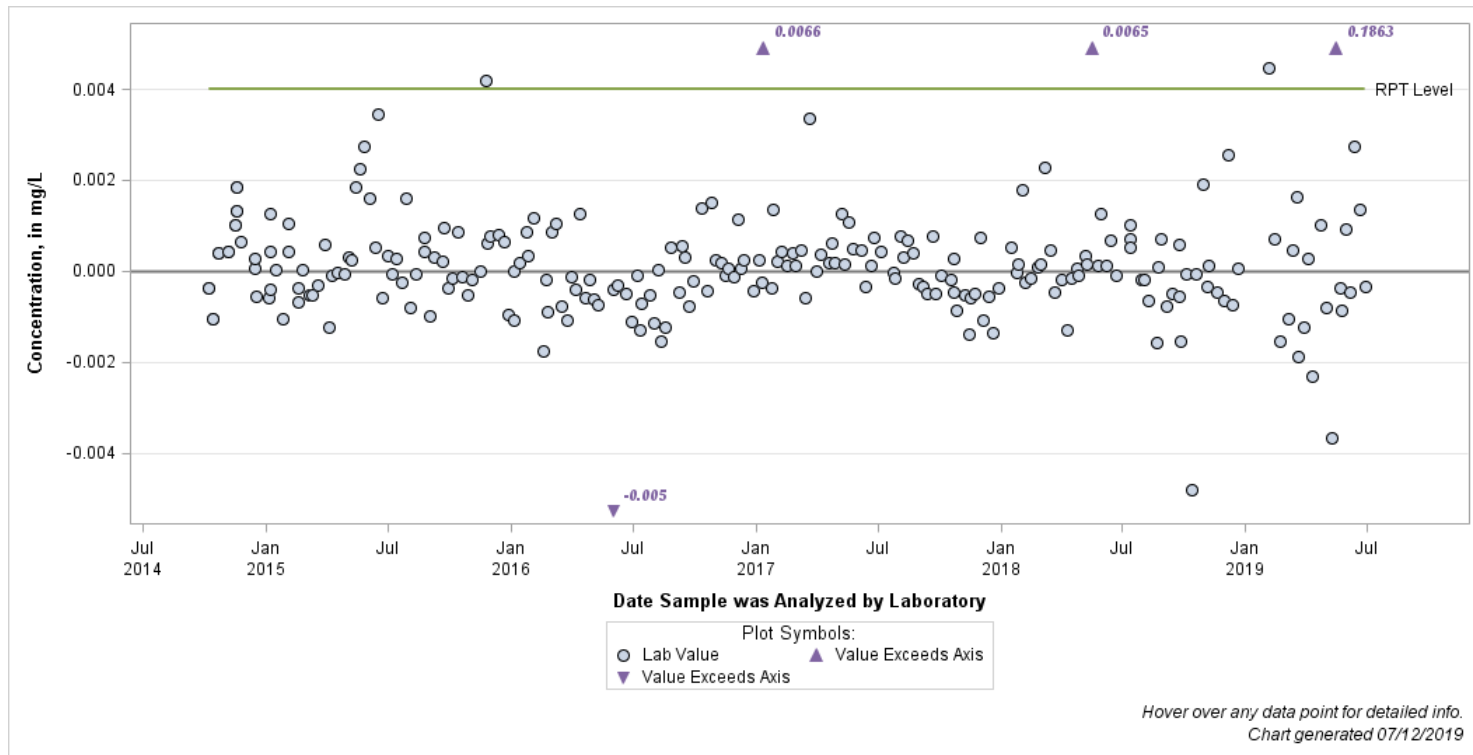


False Positive Rate for Orthophosphate (PO4 as P), FIL, DA

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Orthophosphate (PO4 as P), FIL, DA	00671PHM01	2014	2	0	0%
		2015	58	0	0%
		2016	51	1	2%
		2017	51	1	2%
		2018	51	1	2%
		2019	32	2	6%

*Hover over any data point for detailed info.
Chart generated 07/12/2019*

**- Phosphorus (as P), FIL, ASF, Kjeldahl -
Blind Blank Results**
Lab: NWQL, PCode: 00666, MCode: KJ005
 Analysis dates: 10/02/14 through 06/20/19
[Open Data Set](#)

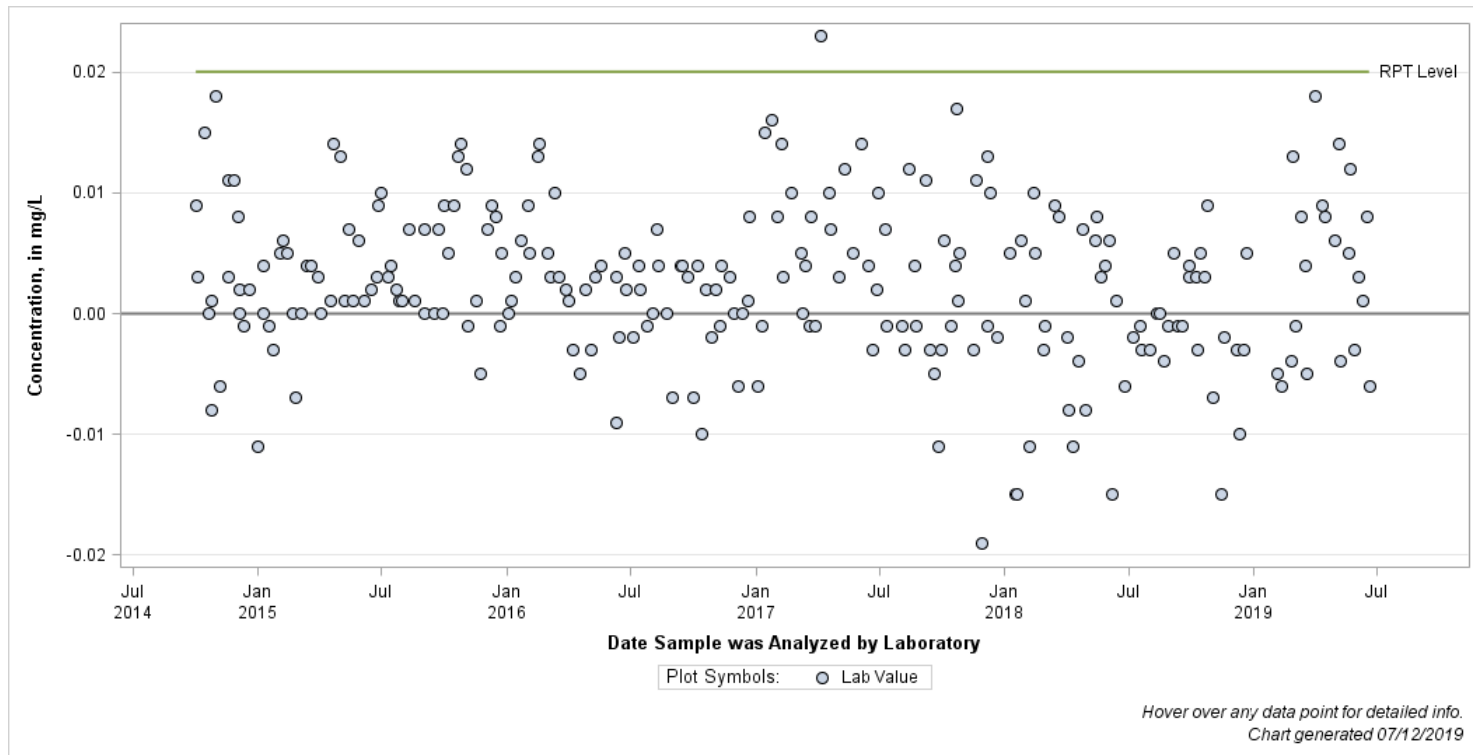


False Positive Rate for Phosphorus (as P), FIL, ASF, Kjeldahl

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Phosphorus (as P), FIL, ASF, Kjeldahl	00666KJ005	2014	5	0	0%
		2015	52	0	0%
		2016	51	0	0%
		2017	51	1	2%
		2018	51	0	0%
		2019	32	0	0%
		<i>*Highlighted if false positive rate > 5 %</i>			

*Hover over any data point for detailed info.
Chart generated 07/12/2019*

- Phosphorus (as P), FIL, CFA, ACD-P, LL -
Blind Blank Results
Lab: NWQL, PCode: 00666, MCode: CL020
 Analysis dates: 10/01/14 through 06/25/19
[Open Data Set](#)

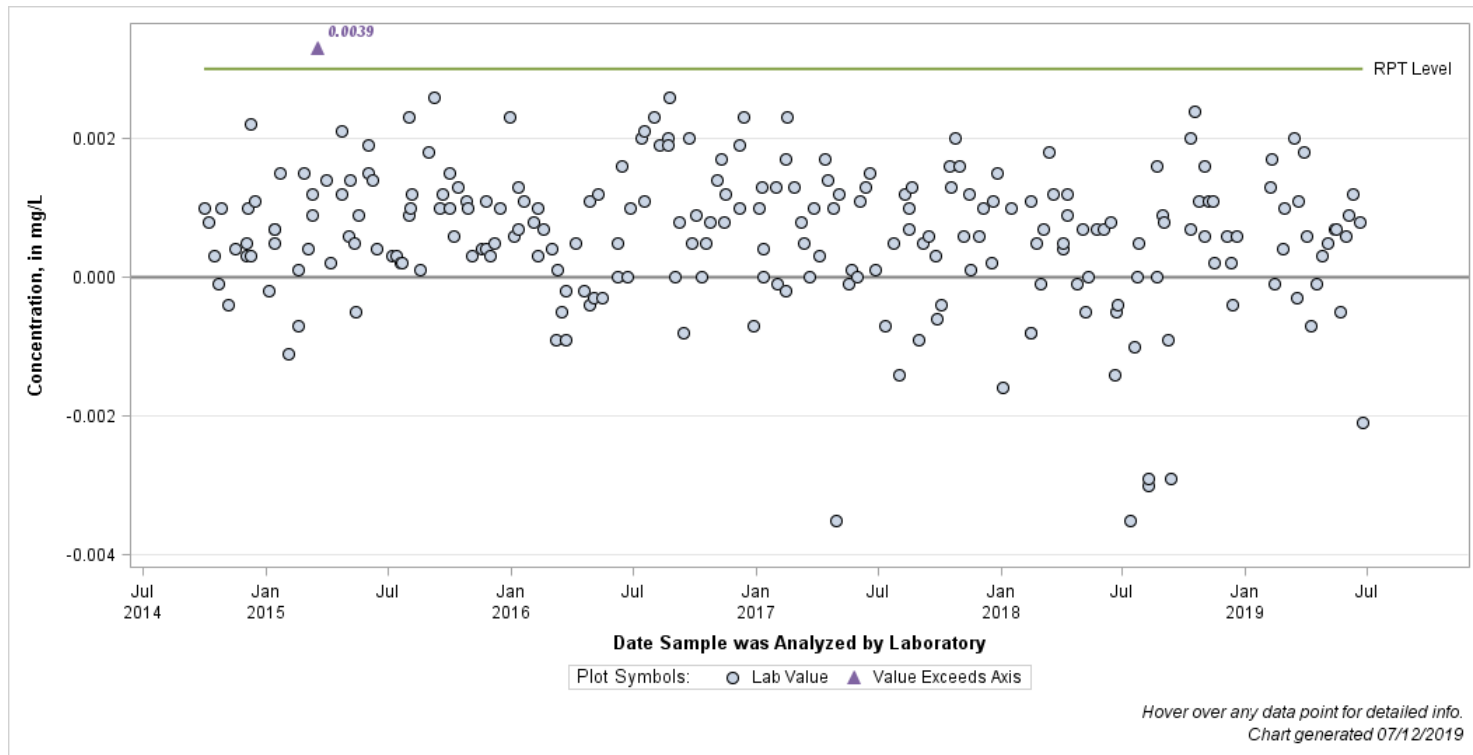


False Positive Rate for Phosphorus (as P), FIL, CFA, ACD-P, LL

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Phosphorus (as P), FIL, CFA, ACD-P, LL	00666CL020	2014	3	0	0%
		2015	52	1	2%
		2016	51	0	0%
		2017	51	0	0%
		2018	51	0	0%
		2019	32	0	0%

**Highlighted if false positive rate > 5 %*

*Hover over any data point for detailed info.
Chart generated 07/12/2019*

- Phosphorus (as P), FIL, CFA, ALK-P -
Blind Blank Results
Lab: NWQL, PCode: 00666, MCode: CL063
 Analysis dates: 10/02/14 through 06/27/19
[Open Data Set](#)

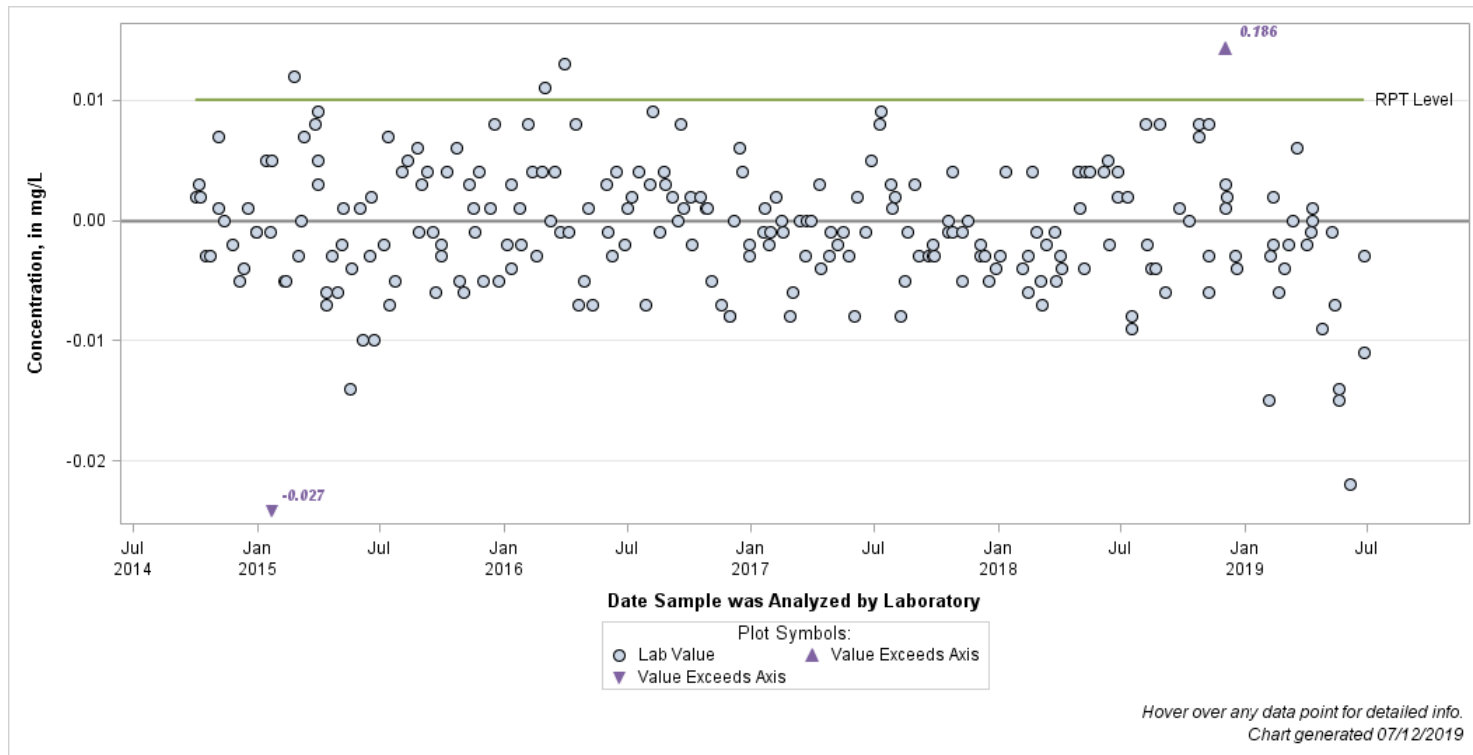


False Positive Rate for Phosphorus (as P), FIL, CFA, ALK-P

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Phosphorus (as P), FIL, CFA, ALK-P	00666CL063	2014	3	0	0%
		2015	52	1	2%
		2016	51	2	4%
		2017	51	0	0%
		2018	51	0	0%
		2019	29	1	3%

**Highlighted if false positive rate > 5 %*

*Hover over any data point for detailed info.
 Chart generated 07/12/2019*

- Phosphorus (as P), UNF, ASF, Kjeldahl -
Blind Blank Results
Lab: NWQL, PCode: 00665, MCode: KJ009
Analysis dates: 10/06/14 through 06/06/19
[Open Data Set](#)

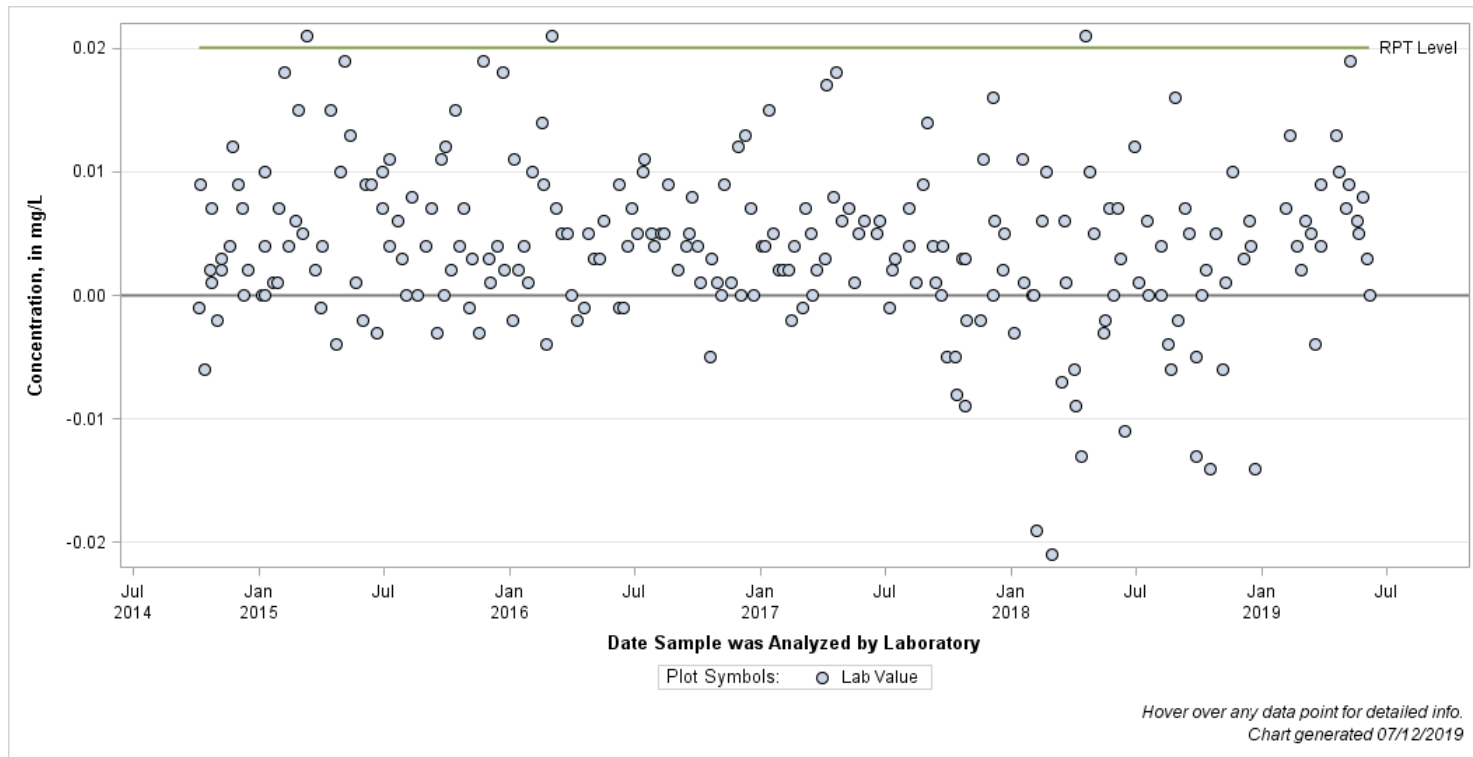

False Positive Rate for Phosphorus (as P), UNF, ASF, Kjeldahl

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Phosphorus (as P), UNF, ASF, Kjeldahl	00665KJ009	2014	5	0	0%
		2015	52	1	2%
		2016	51	1	2%
		2017	51	0	0%
		2018	51	1	2%
		2019	29	0	0%
		<i>*Highlighted if false positive rate > 5 %</i>			

Hover over any data point for detailed info.
Chart generated 07/12/2019


- Phosphorus (as P), UNF, CFA, ACD-P, LL -

Blind Blank Results

Lab: NWQL, PCode: 00665, MCode: CL021

Analysis dates: 10/02/14 through 06/11/19

[Open Data Set](#)

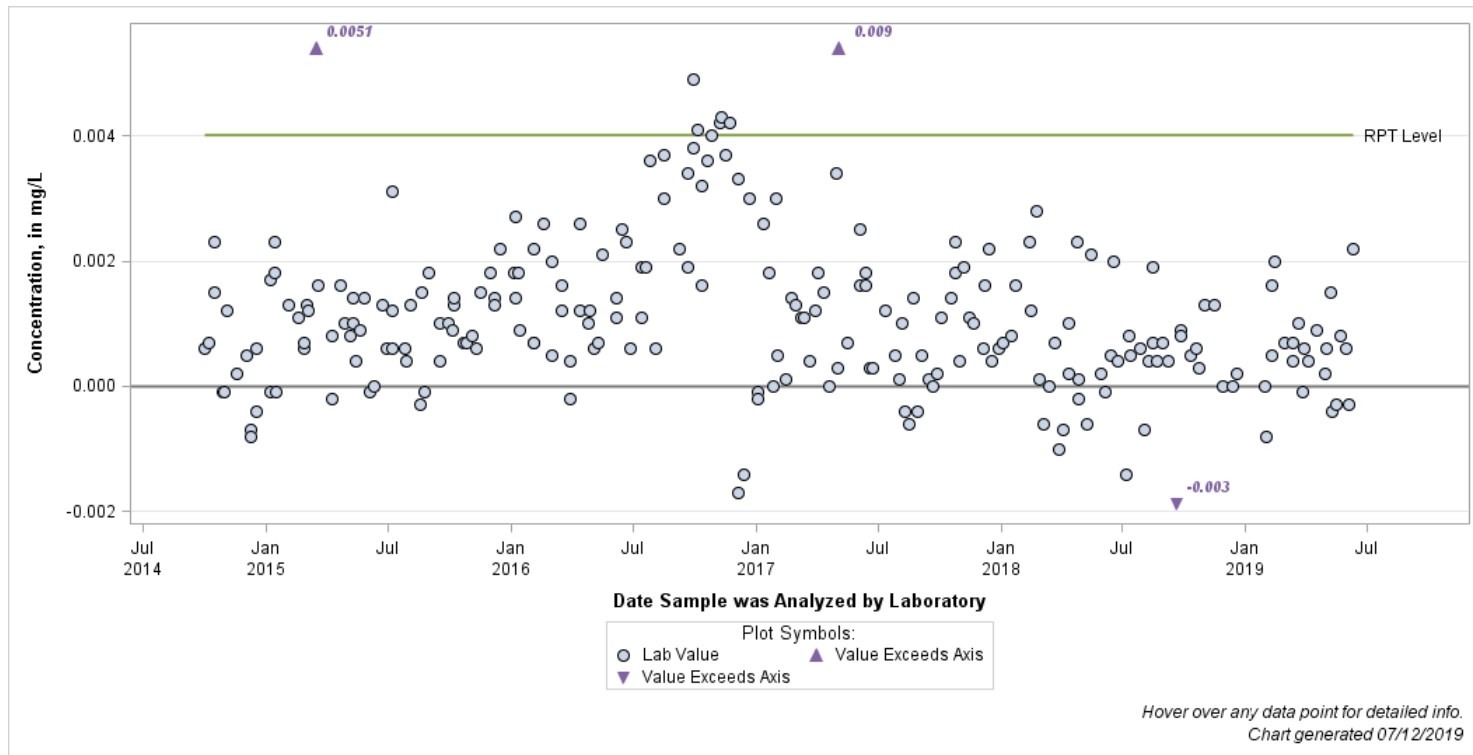


False Positive Rate for Phosphorus (as P), UNF, CFA, ACD-P, LL

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Phosphorus (as P), UNF, CFA, ACD-P, LL	00665CL021	2014	3	0	0%
		2015	52	1	2%
		2016	51	2	4%
		2017	51	4	8%
		2018	51	0	0%
		2019	29	0	0%

Hover over any data point for detailed info.
 Chart generated 07/12/2019

- Phosphorus (as P), UNF, CFA, ALK-P, ACD -
Blind Blank Results
Lab: NWQL, PCode: 00665, MCode: AKP01
Analysis dates: 10/07/14 through 06/27/19
[Open Data Set](#)

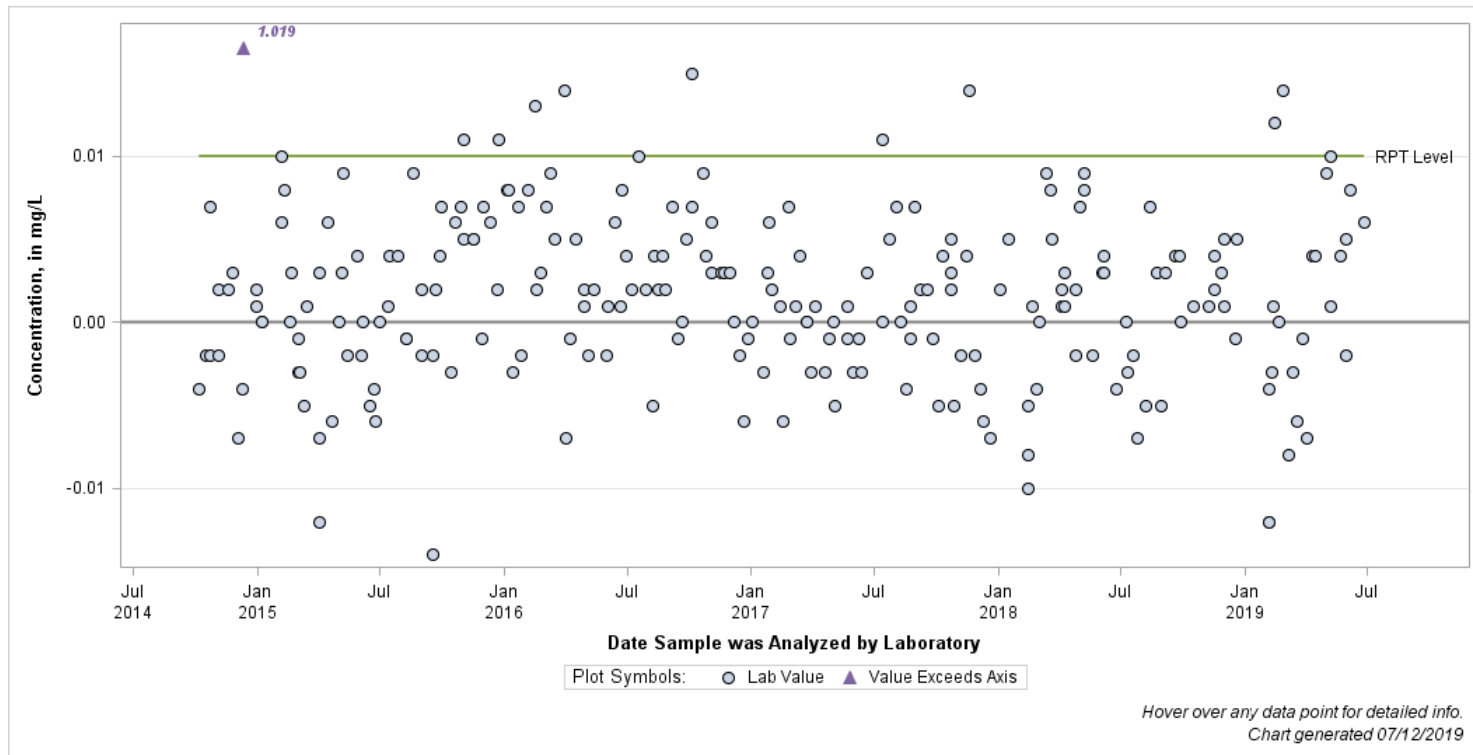

False Positive Rate for Phosphorus (as P), UNF, CFA, ALK-P, ACD

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Phosphorus (as P), UNF, CFA, ALK-P, ACD	00665AKP01	2014	2	0	0%
		2015	52	1	2%
		2016	51	5	10%
		2017	51	1	2%
		2018	51	1	2%
		2019	29	2	7%
		*Highlighted if false positive rate > 5%			

Hover over any data point for detailed info.
Chart generated 07/12/2019


- Total Nitrogen (NH3+NO3+NO2+org N as N), FIL, CFA, ALK-P -

Blind Blank Results

Lab: NWQL, PCode: 62854, MCode: CL063

Analysis dates: 10/02/14 through 06/26/19

[Open Data Set](#)

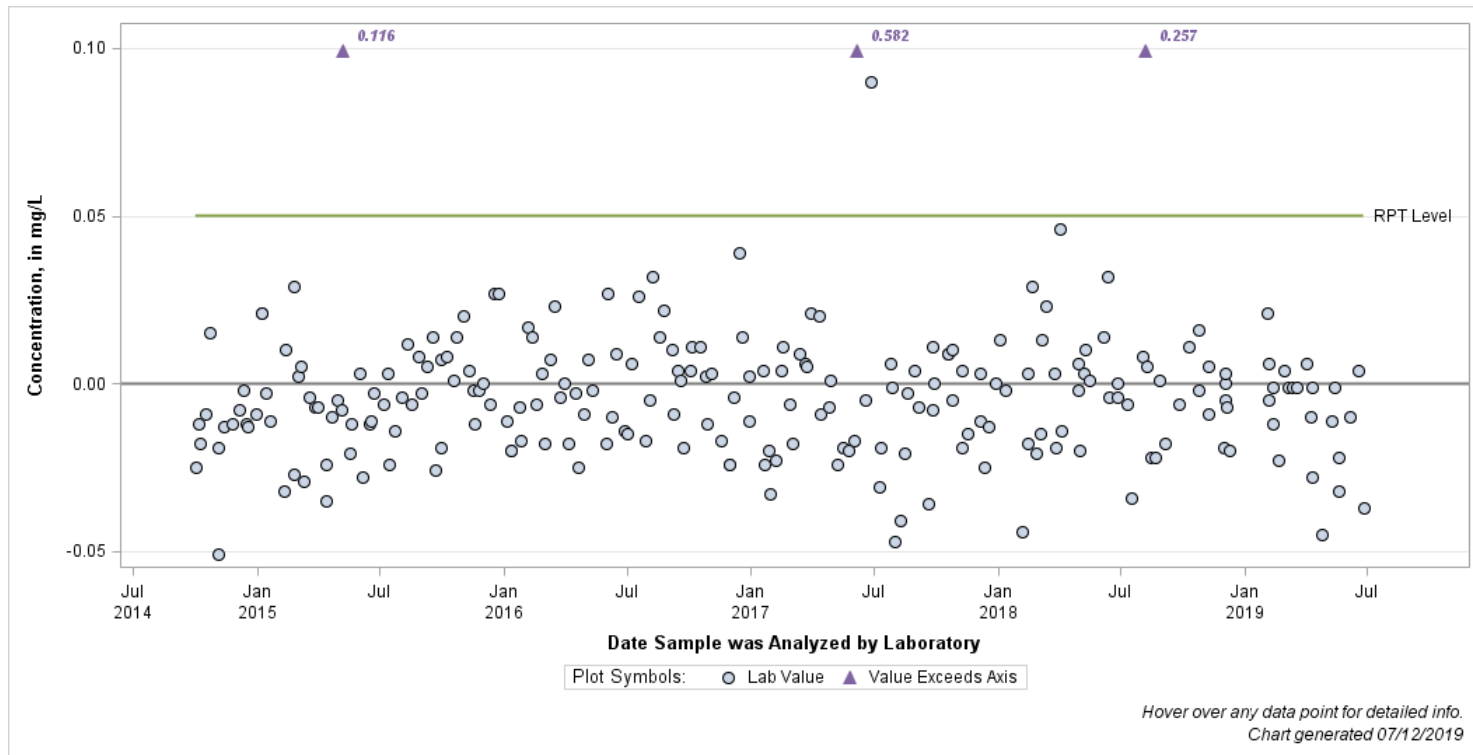

False Positive Rate for Total Nitrogen (NH3+NO3+NO2+org N as N), FIL, CFA, ALK-P

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Total Nitrogen (NH3+NO3+NO2+org N as N), FIL, CFA, ALK-P	62854CL063	2014	3	0	0%
		2015	52	1	2%
		2016	51	0	0%
		2017	51	2	4%
		2018	51	1	2%
		2019	29	0	0%

*Highlighted if false positive rate > 5%

Hover over any data point for detailed info.
Chart generated 07/12/2019


- Total Nitrogen (NH3+NO3+NO2+org N as N), UNF, CFA, ALK-P, ACD -

Blind Blank Results

Lab: NWQL, PCode: 62855, MCode: AKP01

Analysis dates: 10/07/14 through 06/27/19

[Open Data Set](#)

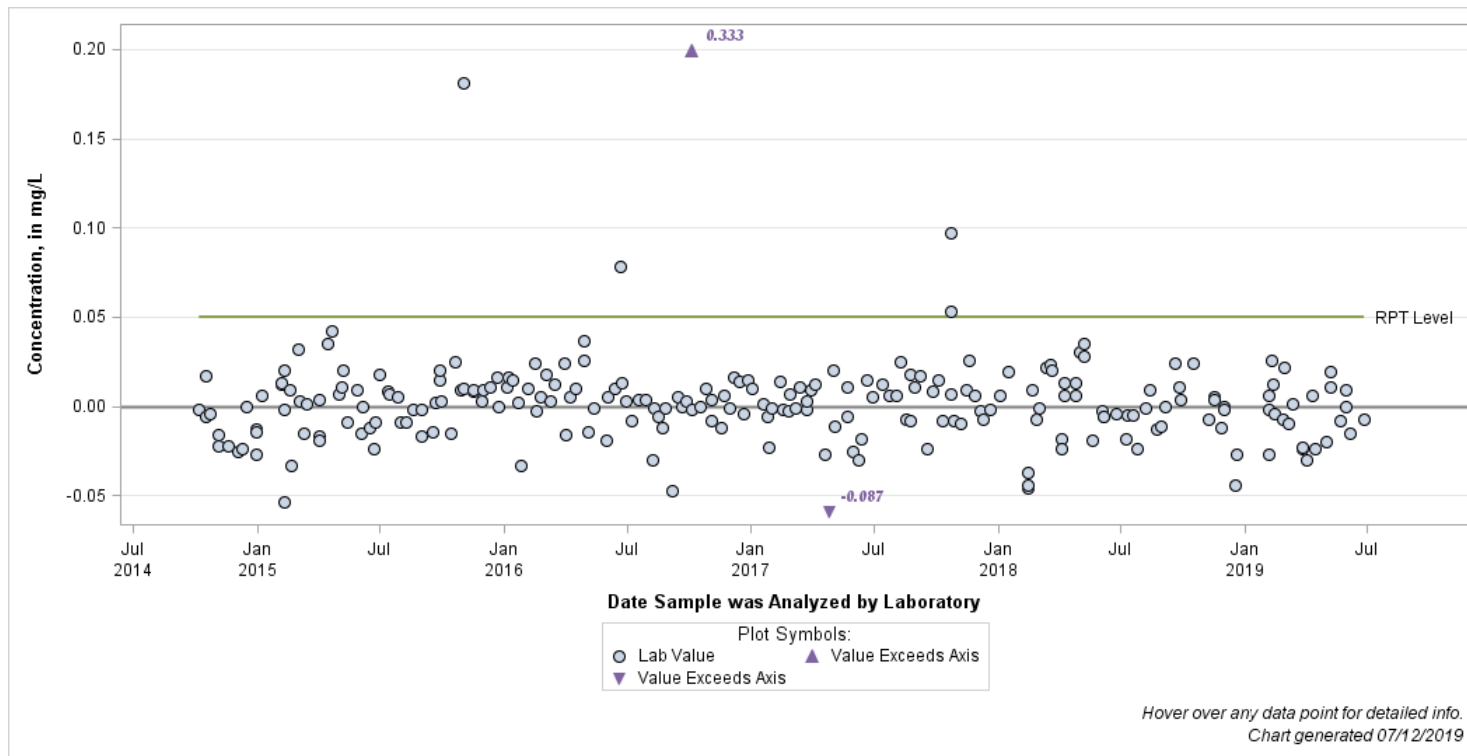

False Positive Rate for Total Nitrogen (NH3+NO3+NO2+org N as N), UNF, CFA, ALK-P, ACD

parmdesc	Pcode Mcode	Water Year	# of Samples	# of False Pos.	*False Positive Rate
Total Nitrogen (NH3+NO3+NO2+org N as N), UNF, CFA, ALK-P, ACD	62855AKP01	2014	2	0	0%
		2015	52	0	0%
		2016	51	3	6%
		2017	51	0	0%
		2018	51	2	4%
		2019	29	0	0%

*Highlighted if false positive rate > 5%

Hover over any data point for detailed info.
 Chart generated 07/12/2019

